



Centralus Health

Laboratory Technical Bulletin

- Cayuga Medical Center Lab
- Schuyler Hospital Lab
- Cayuga Park Lab
- Arnot Ogden Medical Center Lab
- Ira Davenport Lab
- [Check all that apply]

Date: 06/04/2026


Effective Date: 06/24/2026

Title: Thyroid Function Cascade Panel

Test(s): Panel to include Thyroid Stimulating Hormone (TSH) with reflexes to Free T4 (FT4), Total T3 (T3), and Thyroid Peroxidase Antibodies (TPO)

Explanation of change: Thyroid Function Cascade will be orderable. See algorithm below.

	New Panel
<i>Perform Site</i>	TSH can be performed at all hospital labs. Reflex tests will be performed at CMC or AOMC.
<i>Test Code</i>	LAB13307
<i>Specimen</i>	SST Yellow (Cayuga & Schuyler), PST Light Green (Arnot & Ira)
<i>Specimen Stability</i>	48 hours
<i>Turnaround Time</i>	Same day for CMC and AOMC

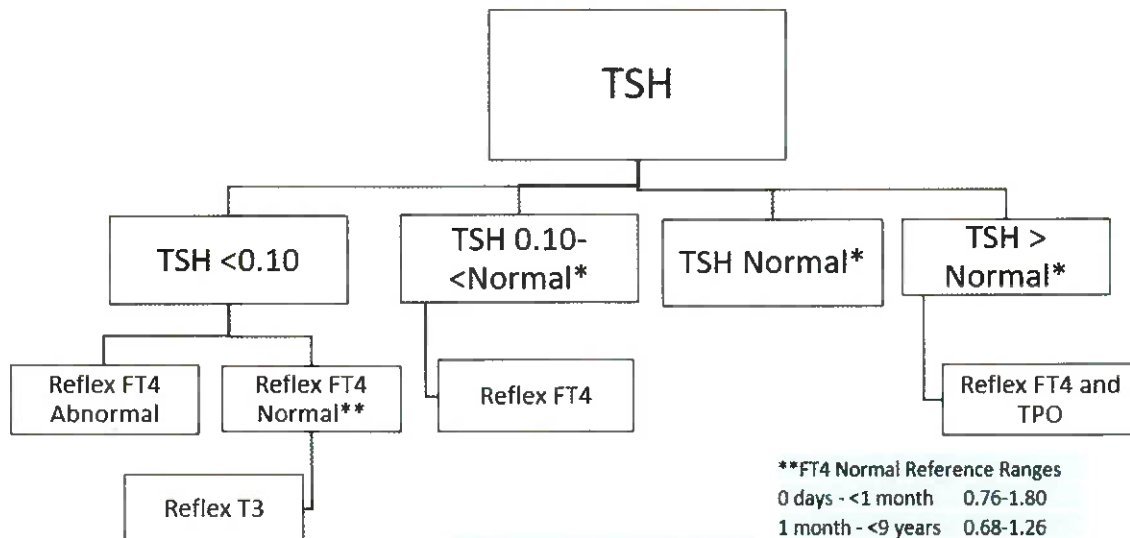

****FT4 Normal Reference Ranges**

0 days - <1 month	0.76-1.80
1 month - <9 years	0.68-1.26
9 years - <11 years	0.75-1.13
11 years - <15 years	0.65-1.05
15 years - <18 years	0.68-1.17
≥18 years old	0.61-1.12

***TSH Normal Reference Ranges**

0 years - <1 year	1.36-8.80
1 year - <3 years	0.85-6.50
≥3 years old	0.45-5.33


 Laboratory Medical Director or Designee

Date 06/17/26